

# Validation Report #029657

Validation Date: 04/03/14

## Summary

Antigen	Dishevelled, Dsh Homolog 1 (Drosophila) (DVL1)
Catalog number	<a href="#">ABIN670671</a>
Supplier	Bioss
Supplier catalog number	<a href="#">bs-0598r</a>
Lot number	140106
Method validated	<a href="#">Immunohistochemistry</a>
Laboratory	<a href="#">Immunohistochemistry Core, NYU Langone</a>
Validation number	<a href="#">029657</a>
Positive Control	<a href="#">Human kidney tubules</a>
Negative Control	<a href="#">Human colon stromal tissue</a>
Notes	While faint, signal is detectable in positive control tissue and not in negative control tissue. Note that staining is expected in colon epithelial cells, and is not expected in kidney glomeruli.



# Full Methods

## **Primary Antibody**

- Antigen: Dishevelled, Dsh Homolog 1 (Drosophila) (DVL1)
- Catalog number: ABIN670671
- Supplier: Bioss
- Supplier catalog number: bs-0598r
- Lot number: 140106

## **Isotype Control Antibody**

- Antibody: Rabbit IgG isotype control
- Supplier: Ventana Medical Systems
- Catalog number: 790-2014
- Lot number: C11245

## **Secondary Antibody**

- Antibody: Biotinylated goat anti-rabbit/anti-mouse (Kit)
- Supplier: Ventana Medical Systems
- Catalog number: 760-091
- Lot number: D07640BA

## **Additional Information**

Detection kit information:

- Type: iView Streptavidin Peroxidase DAB
- Supplier: Ventana Medical Systems
- Catalog number: 760-091
- Lot number: D07640A

## **Controls**

- Positive control: Human kidney tissue stained with antibody
- Negative control: Human colon tissue stained with antibody
- Isotype control: Human kidney tissue stained with isotype control
- Secondary only control: Human kidney tissue stained with secondary antibody only

## **Protocol**

Immunohistochemistry was performed on a Ventana NEXes automated platform; instrument manufacturer specific reagents are italicized.

1. Slides were preheated in convection oven at 60°C for 30 min
2. Deparaffinization procedure:
  - 3 changes of Xylene, 5 min each
  - 3 changes of 100% Ethanol, 3 min each
  - 3 changes of 95% Ethanol, 3 min each
  - Rinsed in distilled water, 3 changes
3. Heat retrieval procedure
  - Slides retrieved in 10.0 mM Citrate, pH6.0 in a 1000W microwave oven (~100°C) for 15 min.
  - Slides were allowed to cool (in citrate) for 30 min.
  - Slides were washed x 3 in Distilled water
4. NEXes instrument procedure, iView DAB paraffin protocol (*abridged*):
  - Slide chamber warmed to 37°C
5. Slides rinsed with *reaction buffer* x3
6. *iView Inhibitor (H2O2)* applied and incubated for 4 min
7. Slides rinsed with *reaction buffer*
8. Antibody Application
  - Primary antibody diluted 1:250 in PBS (100 microliter applied/slide)
  - Ventana Isotype control applied neat
  - Slides Incubated overnight at room temperature (~12 hours ~25°C)

9. Slides rinsed with *reaction buffer* x3
10. *iView Biotinylated IgG* applied and incubated for 8 min
11. Slides rinsed with *reaction buffer*
12. *iView Streptavidin-Horseradish Peroxidase* applied and incubated for 8 min
13. Slides rinsed with *reaction buffer*
14. *iView DAB/H<sub>2</sub>O<sub>2</sub>* applied and incubated for 8 min
15. Slides rinsed with *reaction buffer*
16. *iView Copper* applied and incubated for 4 min
17. Slides rinsed with *reaction buffer*
18. Slides washed in Dawn Detergent/tap water
19. Counterstain Procedure
  - Hematoxylin (Leica 560 MX) 30 sec
  - Slides washed in tap water, 1 min
  - Decolorized (10% Acetic Acid in 70% ethanol), 1 min
  - Slides washed in tap water, 1 min
  - Bluing (Austin Clear Ammonia), 1 min
  - Slides washed in tap water, 1 min
20. Dehydration/cover slipping procedure:
  - 3 changes of 95% Ethanol, 3 min each
  - 3 changes of 100% Ethanol, 3 min each
  - 3 changes of Xylene, 5 min each
  - Mounted with Permount
21. Imaging: Leica SCN 400F Whole Slide Scanner with Digital Image Hub and Leica Slidepath software

### **Experimental Notes**

- Step 1: Heated tissue 60°C for 30 minutes; manufacturer heats for 45 minutes.
- Step 2: No ethanol wash was performed during deparaffinization; manufacturer includes 1 wash of 80% ethanol for 3 minutes.
- Step 3.1: Slides were heated for 15 minutes; manufacturer provides a range of 15-20 minutes.
- Step 3.2: Slides were cooled for 30 minutes; manufacturer cools for 20 minutes.
- Step 4: Italicized reagents and incubation time are fixed instrument parameters.
- Step 5: Secondary species-specific serum block not used; manufacturer blocks with 5% normal goat serum for 2 hours.
- Step 8.1: Antibody diluted in PBS at 1:250; manufacture did not recommend diluent or dilution.
- Step 8.2.1: Primary antibody incubated at room temperature overnight; manufacturer incubates overnight 4°C with agitation.

## Figures

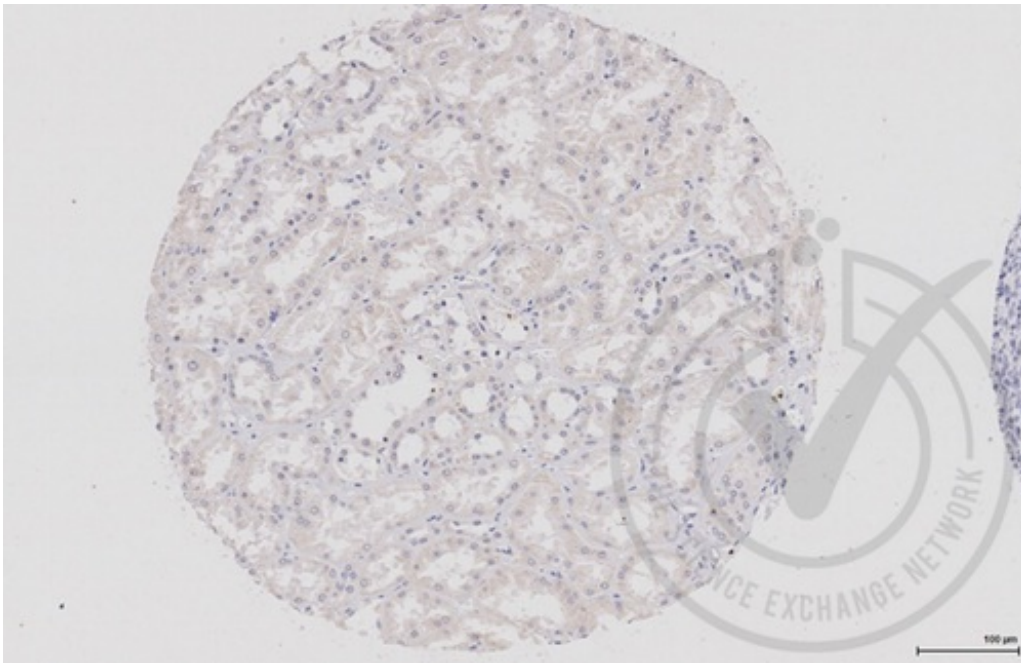


Figure 1: Human kidney tissue stained with anti-DVL1 (brown) and counterstained with hematoxylin.

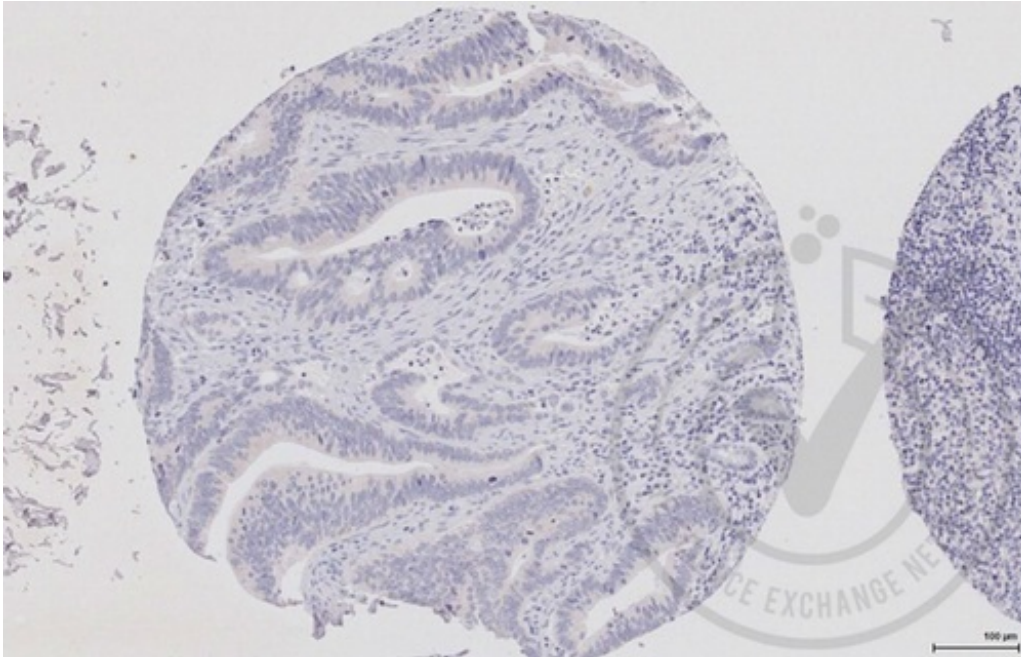


Figure 2: Human colon tissue stained with anti-DVL1 (brown) and counterstained with hematoxylin.

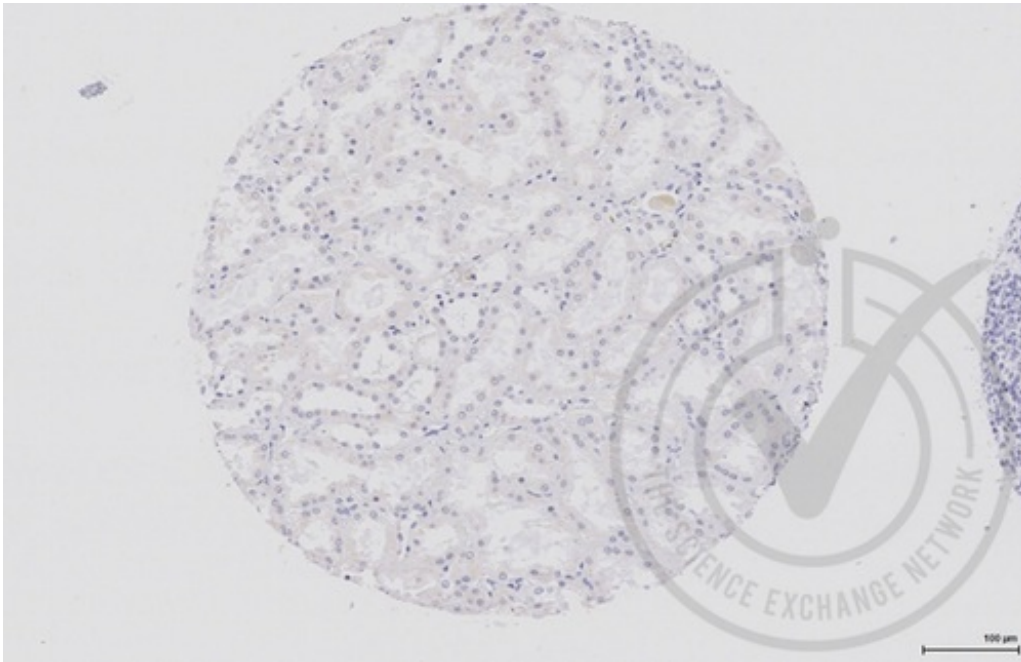


Figure 3: Human kidney tissue stained with isotype control antibody (brown) and counterstained with hematoxylin.

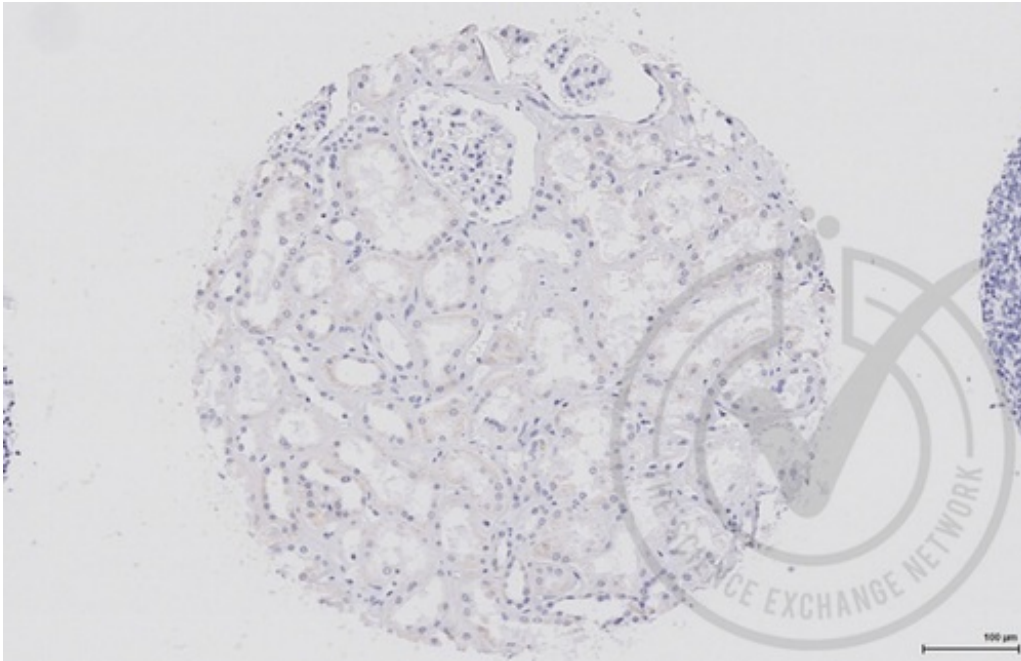


Figure 4: Human kidney tissue stained with secondary only (brown) and counterstained with hematoxylin.